



Welch Allyn

Lamps

Maximise performance
for the life of your product

WelchAllyn

Advancing Frontline Care™

Integrity

LAMP NUMBER	REPLACEMENT LAMP	PRODUCT	LAMP NUMBER	REPLACEMENT LAMP	PRODUCT
00200-U NHSSC Code No FFC023		20100, 21600, 235*, 26000*, 26030, 40510*, 41000, 42700*, 380 SERIES, 385 SERIES, 38800, 395 SERIES, 77900*	03800-U		11800*, 11810, 11820
01200-U NHSSC Code No FFC024		12500, 12500-D, 12500-Y, 12500-DY	03900-U NHSSC Code No FFC026		11110*, 12810
01300-U		28000, 76000*, 77700*	04200-U NHSSC Code No FFC014		48604*, 48614*, 48624*, 48634*, 48704
03000-U NHSSC Code No FFC008		11600*, 11605*, 11610*, 11710, 12400, 18000*, 47300	04400-U NHSSC Code No FFC020		11400*, 11411*, 11470, 11475
03100-U NHSSC Code No FFC007		20000, 20200, 20202, 21700, 25000*, 25020, 25200*, 26530, 26538, 27000, 27050, 28100, 41100, 43300, 73500	04430-U		44304, 44314
03400-U NHSSC Code No FFC012		21110*, 21111*, 24000*, 24011*, 24020*, 24031, 27200, 27250, 41110, 73550	04450-U		44504, 44514
03500-U		23104	04700-U		634, 664, 674, 680, 684* 690, 692, SERIES SIZES 0-1, 694* SERIES SIZES 1-2
03600-U		60500	04800-U		40415, 634, 640*, 664, 674, 680, 684* SERIES SIZES 2-4, 640* SERIES SIZE 1, 690, 692, 694* SERIES SIZES 3-4


To help preserve the integrity of your Welch Allyn products, using genuine Welch Allyn lamps is vital.

Using a Welch Allyn lamp is critical to achieving the optimum performance in use as all our devices are designed as one unit. Using lamps which are not manufactured by Welch Allyn can lead to an inferior performance.

Our testing shows that some generic lamps lose about 50% of their initial light output after only six hours of use, while our lamps sustain close to their initial light output up to four times longer.

For ease of identification, genuine Welch Allyn lamps will always have the re-ordering information stamped or engraved on all units.

Welch Allyn continues to produce lamps for its complete range of products, to ensure that even its older products continue to provide optimal performance.

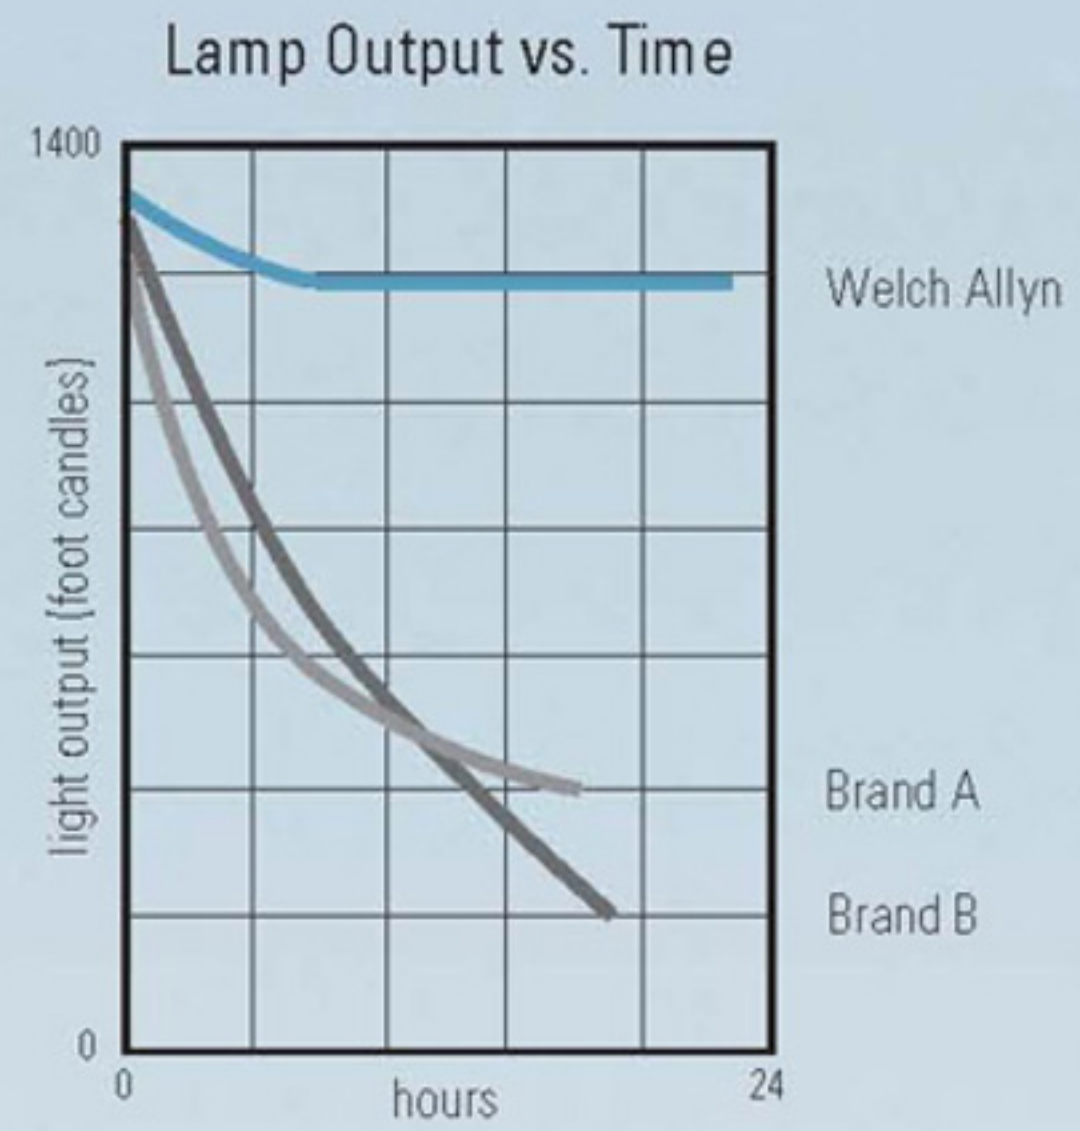

Remember – you can't be sure it is Welch Allyn unless you buy from Welch Allyn or through the NHS Supply Chain

LAMP NUMBER	REPLACEMENT LAMP	PRODUCT	LAMP NUMBER	REPLACEMENT LAMP	PRODUCT
04900-U		11620*, 11630*, 11720, 11730, 11735	08200-U NHSSC Code No FFC016		18200*, 18235*, 18245
06000-U NHSSC Code No FFC015		60713, 60803*, 60804*, 60813, 60814, 60815	08300-U NHSSC Code No FFC025		18300
06200-U		23000*, 23020*, 23040*, 23300	08400-U		93300
06400-U		44204	08500-U NHSSC Code No FFC021		20524H, 20524S, 20514H, 20514S
06500-U NHSSC Code No FFC013		23810, 23820	08800-U NHSSC Code No FFC022		78814
07200-U		17200	09500-U NHSSC Code No FFC018		49504
07600-U NHSSC Code No FFC017		76600	09800-U		88004A, 89004A
07800-U		73200*, 73210, 78000	NATIONAL HEALTH SERVICE SUPPLY CHAIN CODE NUMBER SHOWN IN BLUE * DENOTES INSTRUMENTS NO LONGER IN PRODUCTION. LAMP IMAGES ARE NOT TO SCALE.		

LAMPS for Products no longer in production

LAMP NUMBER	REPLACEMENT LAMP	PRODUCT	LAMP NUMBER	REPLACEMENT LAMP	PRODUCT
00900-U		10600, 110, 121, 17600, 17610	03300-U		11500, 11511
01400-U		77800	03700-U		18100
02000-U		45003	04100-U		48404, 48414
02200-U		22900	04500-U		18010
02500-U		46003	04600-U		17710
02600-U		49003	06100-U		48434
02800-U		2.5V 190 VAG ILLUMINATION SYSTEMS	06300-U NHSSC Code No FFC019		44104, 44114
02900-U		2.5V 290 VAG ILLUMINATION SYSTEM (78500)	08100-U		48104
03100-1	REPLACED BY 03100-U	25000, 25200	09600-U		49604, 47104

REPLACEMENT BATTERIES

As well as using lamps manufactured by Welch Allyn to help preserve the integrity of your Welch Allyn products, using genuine Welch Allyn batteries is also recommended.

BATTERY NUMBER	BATTERY	PRODUCT
72200		NiCad Handle for desk charger 71670
72300		NiCad Handle 71020-A 71020-C

WelchAllyn®

Advancing Frontline Care™